



SimpliNano™ spectrophotometer

SimpliNano is a simple-to-use microvolume spectrophotometer for straightforward concentration and purity measurements of nucleic acids and proteins (Fig 1).

SimpliNano uses a built-in sample port that can be used with a variety of common lab chemicals and has no moving parts, making it reliable, easy-to-use, and clean. It has a fixed pathlength that does not require any calibration. The ability to pipette volumes down to 1 μ l directly onto the sample port eliminates the need for cuvettes or other sampling tools. After measurement, the sample can either be easily recovered with a pipette or quickly discarded by wiping the sample port clean for the next measurement.

SimpliNano is preprogrammed with a range of preset methods for the quantitation of nucleic acids and direct UV proteins, with graphical display of resulting wavescans. The SimpliNano direct user interface means that there is no need for a computer, so fast instrument start-up is possible.

SimpliNano offers the following benefits:

- **Simple sample handling:** Built-in sample port (Fig 2) with one fixed pathlength means that samples can be added and removed without the need for time-consuming pathlength calibration. SimpliNano contains no moving parts, which contributes to excellent instrument reproducibility and low maintenance.
- **Low sample volumes:** Reduce sample loss and eliminate the need for dilution by using low volumes of 1 to 5 μ l for sample measurement. The sample can either be recovered or simply wiped away after measurement.
- **Built-in life science methods:** Measures nucleic acid concentrations at 260 nm, protein concentrations at 280 nm, and provides 230/260 and 260/280 ratios for determining sample purity. Wavescan plots from 220 nm to 330 nm can be achieved for nucleic acids and from



Fig 1. SimpliNano is an easy-to-use, low-maintenance spectrophotometer designed for analysis of low volumes of nucleic acid and protein samples, shown here with printer option.

250 nm to 350 nm for protein. The methods include options for background correction at 320 nm and 340 nm.

- **Flexible instrument control:** Use as either a stand-alone instrument using its large, built-in screen for quick measurements or operate from a PC with optional Datrys software.
- **Choice of data output:** Output to any suitable PC via a USB cable, to an optional integrated printer, or to a USB stick.

Technical specifications for SimpliNano are given in Table 1.

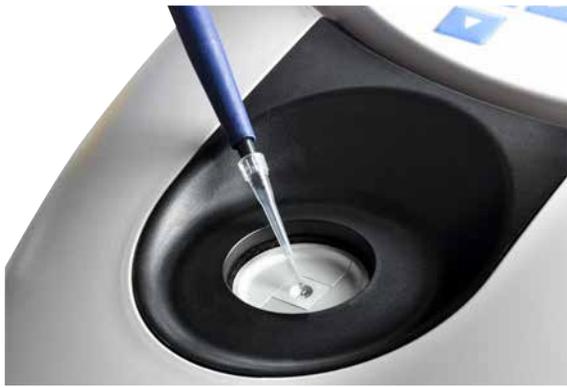


Fig 2. The built-in sample port allows direct application of 1 to 5 μl volumes of sample.

Table 1. Technical specifications for SimpliNano

Wavelength range	190 to 1100 nm
Pathlength	0.5 mm
Minimum sample size	1 μl
Absorbance range	-0.3 to 2.5 Abs. units (10 mm equivalent to 50 Abs. units)
Spectral bandwidth	5 nm
Light source	Xenon
Detector type	CCD array
Data output to PC	Via USB cable (standard); USB memory stick (standard); integrated printer (optional)
Dimensions	260 \times 390 \times 130 mm
Weight	Approx. 3 kg
Power requirements	90 to 250 V, 50/60Hz, max 30 VA

Assays

Nucleic acids

SimpliNano allows you to measure the concentration and purity of nucleic acids in a variety of units ($\mu\text{g}/\text{ml}$, $\text{ng}/\mu\text{l}$, and $\mu\text{g}/\mu\text{l}$) and also, to correct for dilution factors where necessary.

The spectrophotometer displays both individual absorbance values and absorbance ratios (260/280 and 260/230) on the screen, along with the sample concentration value. The results can be printed immediately with the on-board printer option. The prestored method includes the option of background correction at 320 nm.

You can examine the UV spectrum (220 to 320 nm) for hybridization, PCR, and sequencing studies or for quantitation of minipreps.

SimpliNano shows excellent linearity with double-stranded DNA (dsDNA) from 4 to 2500 $\mu\text{g}/\text{ml}$ (Fig 3). This large linear dynamic range and high reproducibility means that you can proceed to the next stage of your workflow with a high degree of confidence in the data.

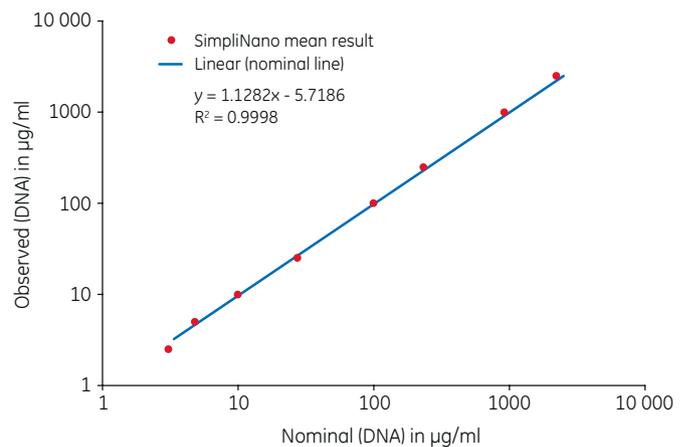


Fig 3. DNA concentration curve (4 to 2500 $\mu\text{g}/\text{ml}$) generated from 10 replicate salmon sperm dsDNA samples (2 μl volumes) measured at 260 nm on SimpliNano. The data in the graph is representative data from one instrument used in the validation study where a total of 6 instruments were tested.

Proteins

SimpliNano can be used to determine the concentration of protein samples in the near UV spectrum at 280 nm due to absorption by the amino acids tyrosine, tryptophan, and phenylalanine. The protein method shows individual absorbance readings for 260 nm and 280 nm and offers background correction at 340 nm. A 260/280 ratio is also provided on the screen. The absorbance at 280 nm varies greatly for different proteins because of their amino acid content and therefore, the specific absorption value for a particular protein must always be determined.

SimpliNano has built-in extinction coefficients for BSA, IgG, and lysozyme, allowing you to select the most appropriate values for your protein sample. You can also input your own extinction coefficients. Figure 4 shows protein linearity over the range of 0.12 to 50 mg/ml.

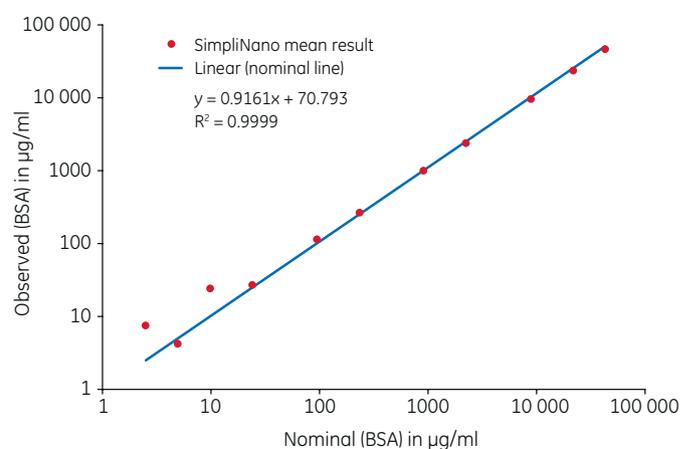


Fig 4. BSA concentration curve (120 to 50 000 $\mu\text{g}/\text{ml}$) generated from a 10% BSA solution. Ten replicate samples (2 μl volumes) were measured at 280 nm on SimpliNano using the BSA program to ensure correct protein coefficient was employed. The data in the graph is representative data from one instrument used in the validation study where a total of 6 instruments were tested.

Sample can be simply removed with a tissue to prevent cross-contamination thus improving data precision. To demonstrate this, sample carryover was determined using high concentrations of protein (BSA) and the results of the carryover experiments are shown in Figure 5.

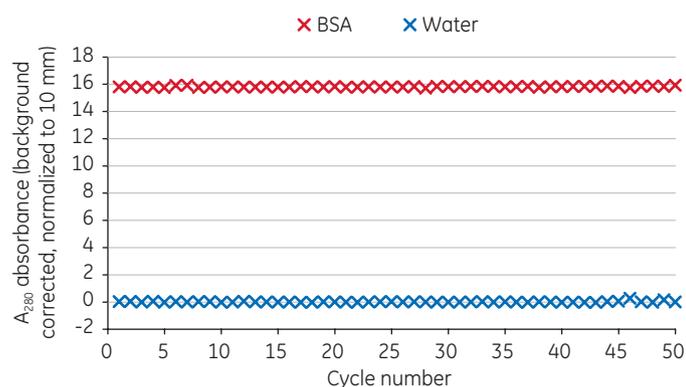


Fig 5. A sample carryover study using 25 mg/ml BSA with successive alternative additions of water and BSA, which was repeated 50 times. The data showed no significant change in absorbance readings throughout the study for the water samples or the BSA samples, indicating that there was no carryover.

Summary

SimpliNano spectrophotometer is an easy-to-use and reliable instrument for measuring nucleic acid and protein samples, without the need for pathlength calibration. SimpliNano offers wavescan plots for nucleic acids and proteins. Samples of 1 to 5 μ l can be pipetted directly onto the sample port for measurement, and then simply recovered using a pipette. In cases where sample recovery is not necessary, the sample port can be quickly and easily wiped clean. This eliminates the need for cuvettes, capillaries, or other sampling tools—just drop, measure, and you're done.

Ordering information

Product	Quantity	Code number
SimpliNano (Worldwide except US and Canada)	1	29-0617-11
SimpliNano with printer (Worldwide except US and Canada)	1	29-0617-12
SimpliNano (North America only)	1	29-0617-13
SimpliNano with printer (North America only)	1	29-0617-14

Related products	Quantity	Code number
NanoVue™ Plus with integrated printer (North America only)	1	28-9569-63
NanoVue Plus with integrated printer (Worldwide except US and Canada)	1	28-9569-66
NanoVue Plus, print via computer (North America only)	1	28-9569-62
NanoVue Plus, print via computer (Worldwide except US and Canada)	1	28-9569-65
NanoVue Plus with wireless connectivity (North America only)	1	28-9569-64
NanoVue Plus with wireless connectivity (Worldwide except US and Canada)	1	28-9569-67
Ultraspec 10 Cell density meter, classic	1	80-2116-30
illustra™ plasmidPrep Mini Spin Kit	50 preps	28-9042-69
illustra GenomiPhi™ V2 DNA Amplification Kit	25 reactions	25-6600-30
illustra triplePrep Kit	50 preps	28-9425-44
illustra HotStart Master Mix	1	25-1500-01
illustra GFX™ PCR DNA and Gel Band Purification Kit	100 preps	28-9034-70
illustra blood genomicPrep Mini Spin Kit	50 preps	28-9042-64
illustra bacteria genomicPrep Mini Spin Kit	50 preps	28-9042-58
illustra tissue and cells genomicPrep Mini Spin Kit	50 preps	28-9042-75
illustra tissue and cells genomicPrep Midi Flow Kit	25 preps	28-9042-73
His Gravitrapp™	10 × 1 ml	11-0033-99
His SpinTrap™	50 × 100 μ l	28-4013-53

Related literature	Code number
UV/Vis spectrophotometers, Brochure	28-9271-31
Spectrophotometers, Handbook	29-0331-82

For local office contact information, visit
www.gelifesciences.com/contact

www.gelifesciences.com/spectros

GE Healthcare UK Limited
Amersham Place
Little Chalfont
Buckinghamshire, HP7 9NA
UK



GE and GE monogram are trademarks of General Electric Company.
GenomiPhi, GFX, GraviTrap, illustra, NanoVue, SimpliNano, and SpinTrap are trademarks of General Electric Company or one of its subsidiaries.

GenomiPhi: For use only as licensed by Qiagen GmbH and GE Healthcare. The Phi 29 DNA polymerase may not be re-sold or used except in conjunction with the other components of this kit. See US patent numbers 5,854,033, 6,124,120, 6,143,495, 6,323,009, 5,576,204, and equivalent patents and patent applications in other countries.

© 2014 General Electric Company—All rights reserved.
First published Apr. 2014

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare which supplies them. A copy of these terms and conditions is available on request. Contact your local GE Healthcare representative for the most current information.

GE Healthcare Bio-Sciences AB
Björkgatan 30
751 84 Uppsala
Sweden

GE Healthcare Europe, GmbH
Munzinger Strasse 5
D-79111 Freiburg
Germany

GE Healthcare Bio-Sciences Corp.
800 Centennial Avenue, P.O. Box 1327
Piscataway, NJ 08855-1327
USA

GE Healthcare Japan Corporation
Sanken Bldg., 3-25-1, Hyakunincho
Shinjuku-ku, Tokyo 169-0073
Japan